

Fig. 1

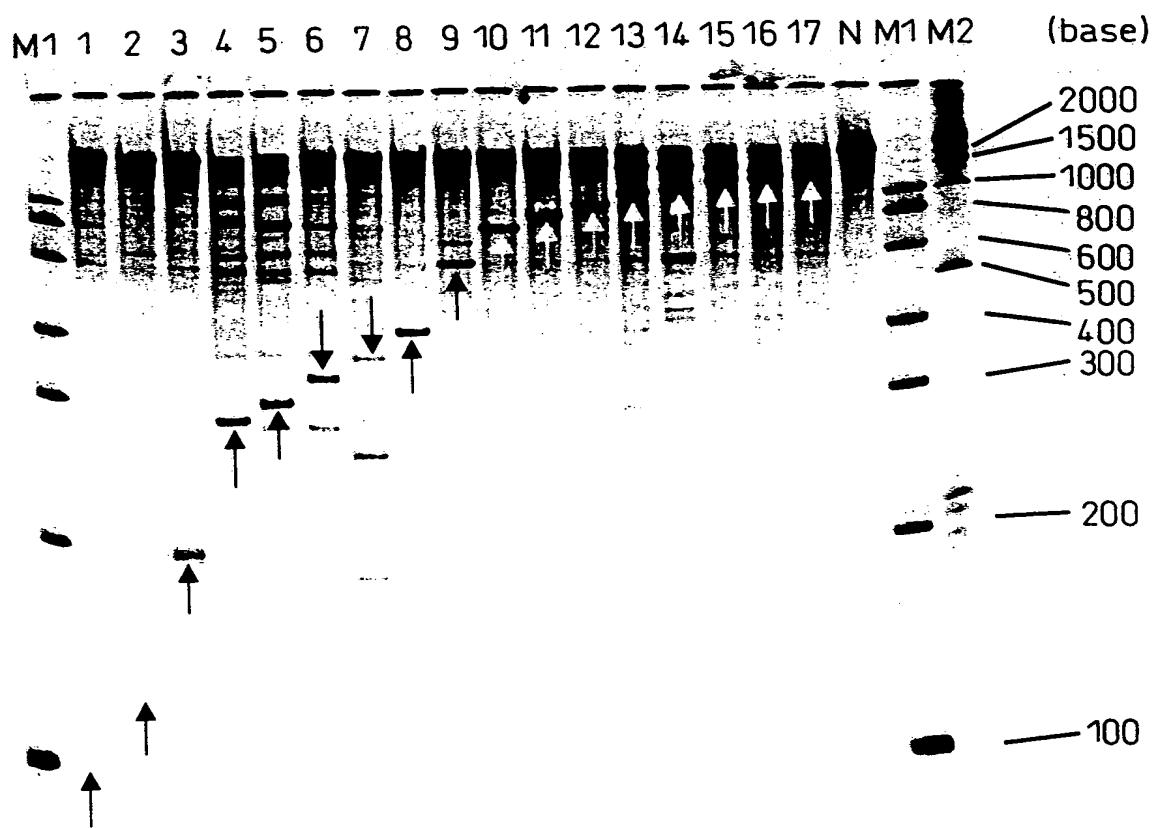


Fig. 2

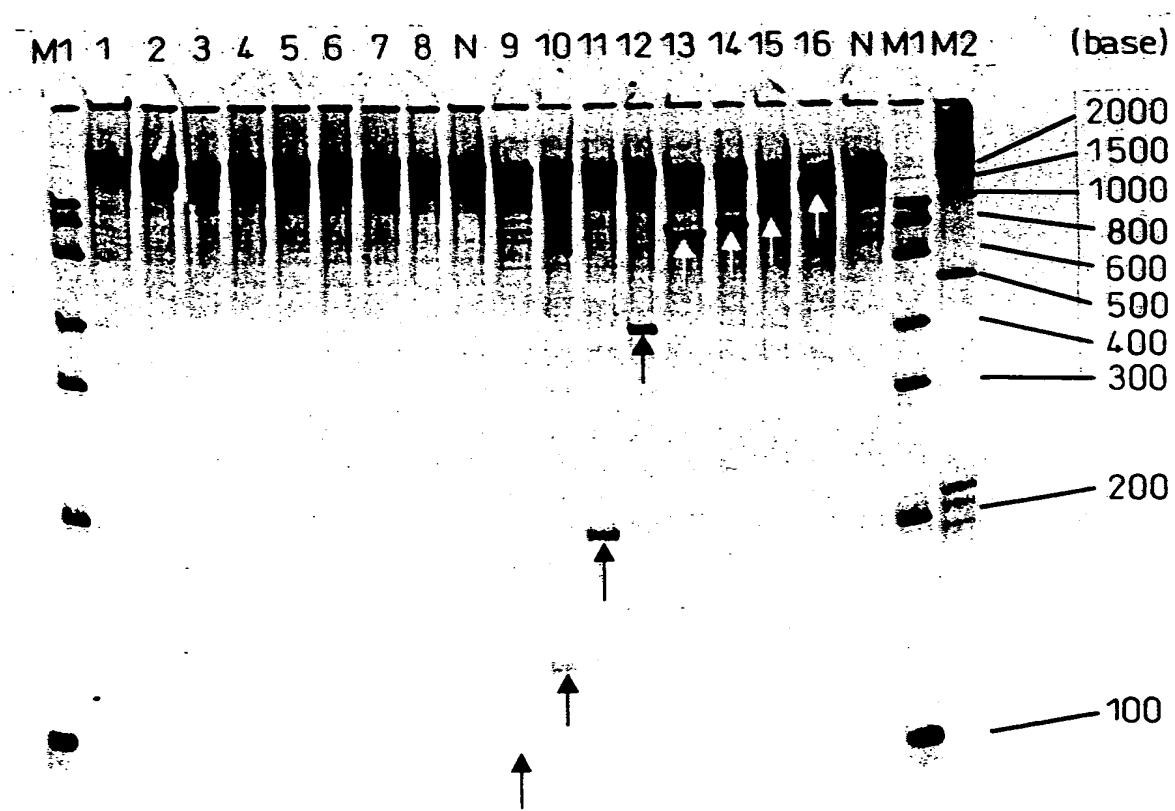


Fig.3


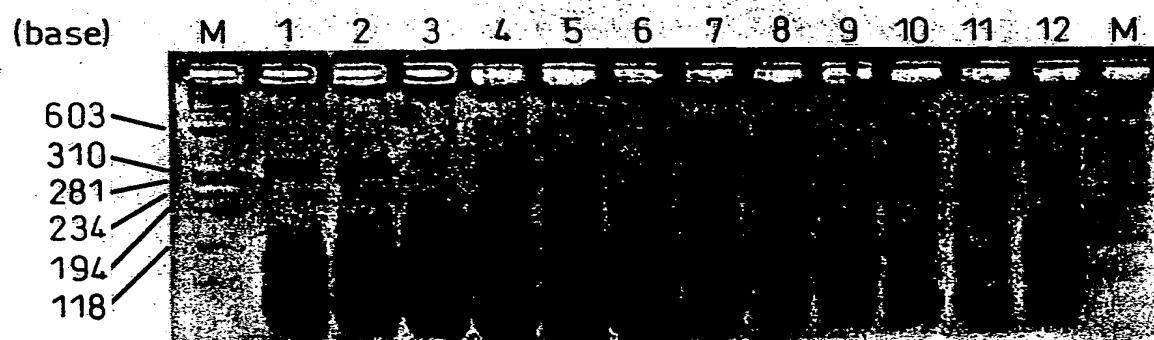


Fig.4

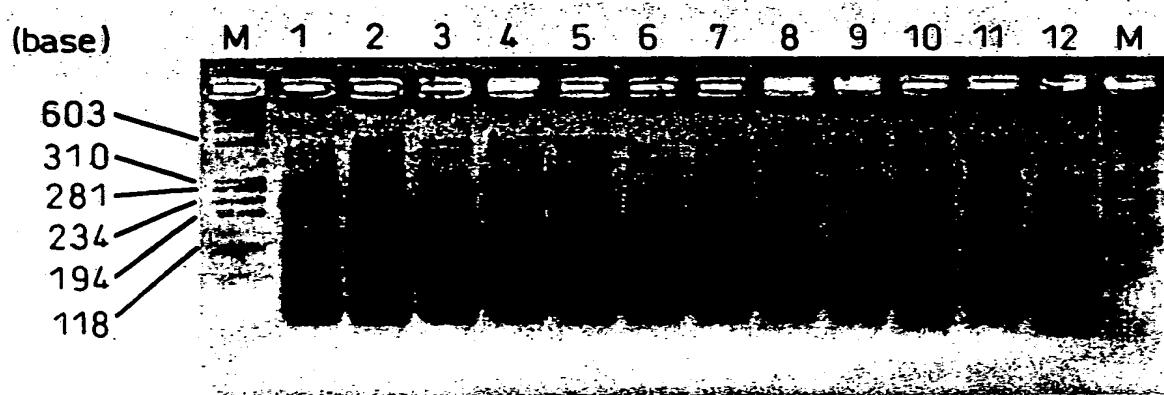

4/5

Fig.5


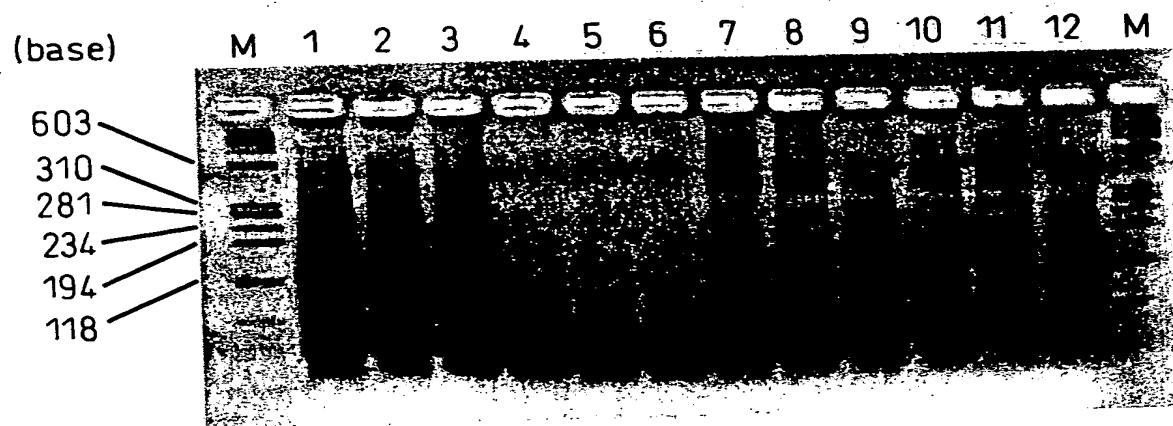


Fig. 6

(A)

FLUORESCENCE PROFILE

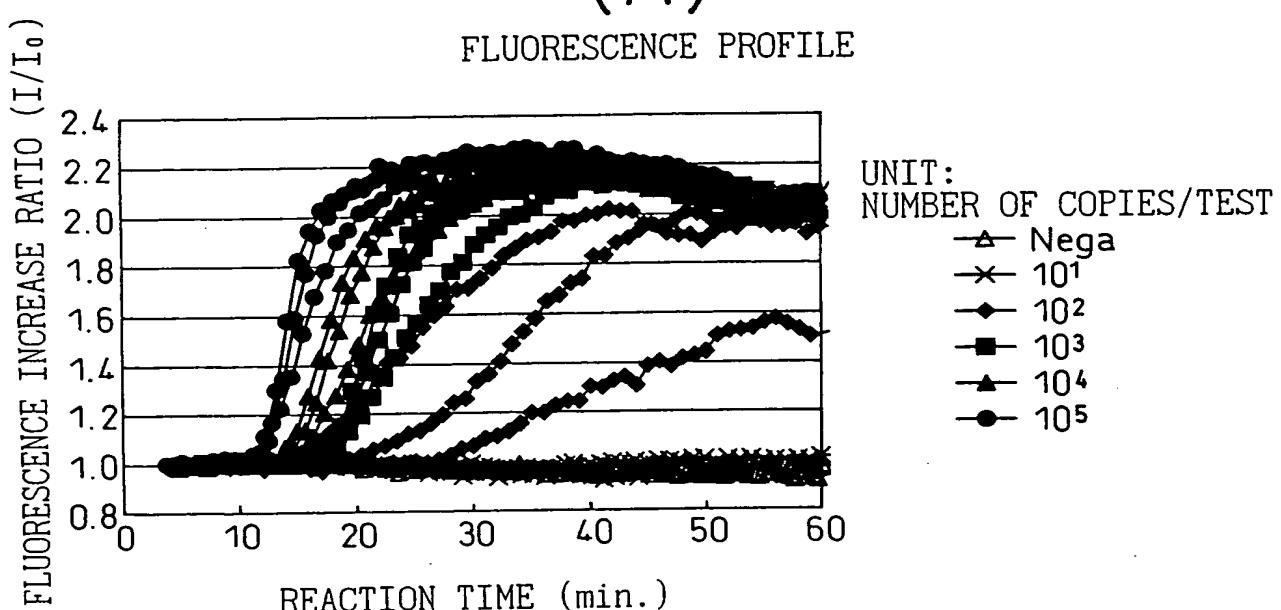

(B)

CALIBRATION CURVE

